



LOC/DME I-SYR 109.9 Chan 36	APP CRS 280°	Rwy Idg TDZE 413 Apt Elev 421
---	------------------------	---

ILS RWY 28 (SA CAT I)
SYRACUSE HANCOCK INTL (SYR)

DME or RADAR required. Requires specific OPSPEC, MSPEC, or LOA approval and use of HUD to DH.		ALSIF-2	MISSED APPROACH: Climb to 1100 then climbing right turn to 3000 direct SYR VORTAC and hold, continue climb-in-hold to 3000.	
ATIS 124.225	SYRACUSE APP CON 126.125 269.125	SYRACUSE TOWER 120.3 239.0	GND CON 121.7 348.6	CLNC DEL 125.05 257.775

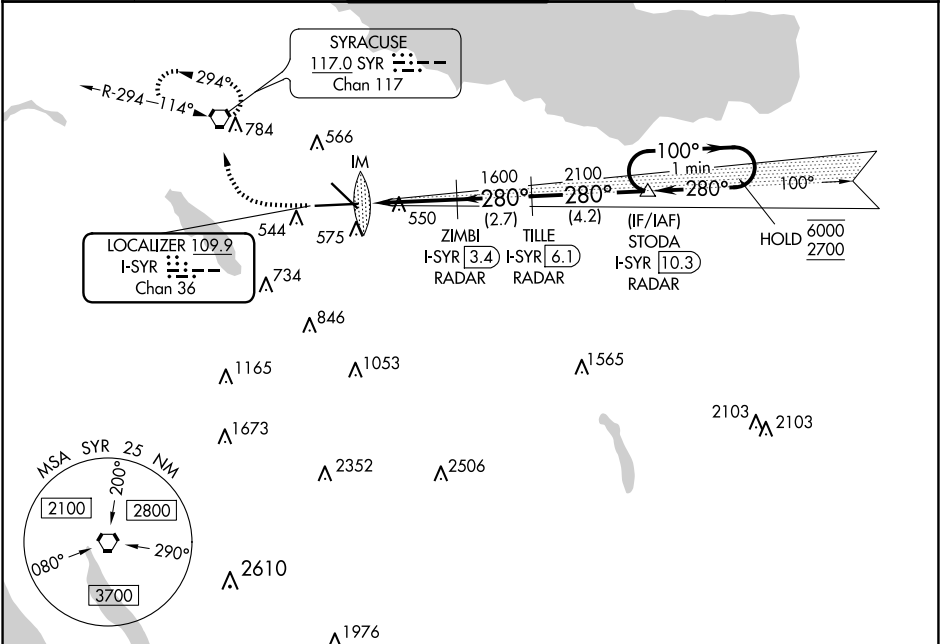

ELEV 421	D	TDZE 413
-----------------	----------	-----------------

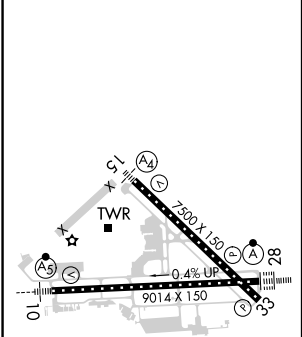

1100	3000	SYR	STODA I-SYR 10.3 RADAR One Minute Holding Pattern	
IM	ZIMBI I-SYR 3.4 RADAR	TILLE I-SYR 6.1 RADAR	I-SYR 10.3 RADAR	100° 6000 280° 2700
1600	1600	2100	280°	GS 3.00° TCH 60
975'	3.6 NM	2.7 NM	4.2 NM	
CATEGORY	A	B	C	D
S-ILS 28	RA 150/14 150 DA 563			

SA CATEGORY I ILS - SPECIAL AIRCREW
& AIRCRAFT CERTIFICATION REQUIRED

NE-2, 20 MAR 2025 to 17 APR 2025

NE-2, 20 MAR 2025 to 17 APR 2025